

1. PERFORMANCE


- 1) Measuring range : 0.05-2.5 %
 Number of pump strokes 1 (100mℓ)
 2) Sampling time : 1.5 minutes/1 pump stroke
 3) Detectable limit : 100 ppm
 4) Shelf life : 3 years
 5) Operating temperature : 0 ~ 40 °C
 6) Temperature compensation : Necessary (See "TEMPERATURE CORRECTION TABLE")
 7) Reading : Graduations printed on the tube are calibrated by Ethylene oxide at 1 pump stroke and Isopropyl alcohol is determined by using a conversion chart.
 8) Colour change : Orange → Dark brown

2. RELATIVE STANDARD DEVIATION

RSD-low : 15 % RSD-mid. : 15 % RSD-high : 5 %

3. CHEMICAL REACTION

Chromium oxide is reduced.



4. CALIBRATION OF THE TUBE

GAS CHROMATOGRAPHY

5. INTERFERENCE AND CROSS SENSITIVITY

Substance	Interference	%	Coexistence
Alcohols FIG.1	Similar stain is produced.		Higher readings are given.
Esters FIG.2	〃		〃
Ketones	〃		〃
Aromatic hydrocarbons	〃		〃
Aliphatic hydrocarbons	Whole reagent is discoloured to Pale brown.	0.5	〃

(NOTE)

Methanol and Ethyl acetate have the same sensitivity as Isopropyl alcohol.

Methyl ethyl ketone has 3/4 sensitivity of Isopropyl alcohol.




FIG.1 Influence of Methanol





FIG.2 Influence of Ethyl acetate

TEMPERATURE CORRECTION TABLE

Conversion Value (%)	Corrected Concentration (ppm)				
	0°C (32°F)	10°C (50°F)	20°C (68°F)	30°C (86°F)	40°C (104°F)
2.5	—	—	2.50	2.10	2.00
2.0	—	—	2.00	1.70	1.62
1.5	—	—	1.50	1.28	1.21
1.0	—	1.43	1.00	0.85	0.80
0.5	1.00	0.62	0.50	0.42	0.38
0.1	0.16	0.14	0.10	0.09	0.08
0.05	0.09	0.06	0.05	0.04	0.03

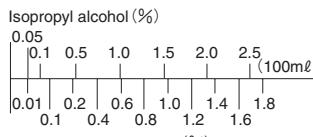

No.122SA Tube reading (%)